USED ON
LA762501D

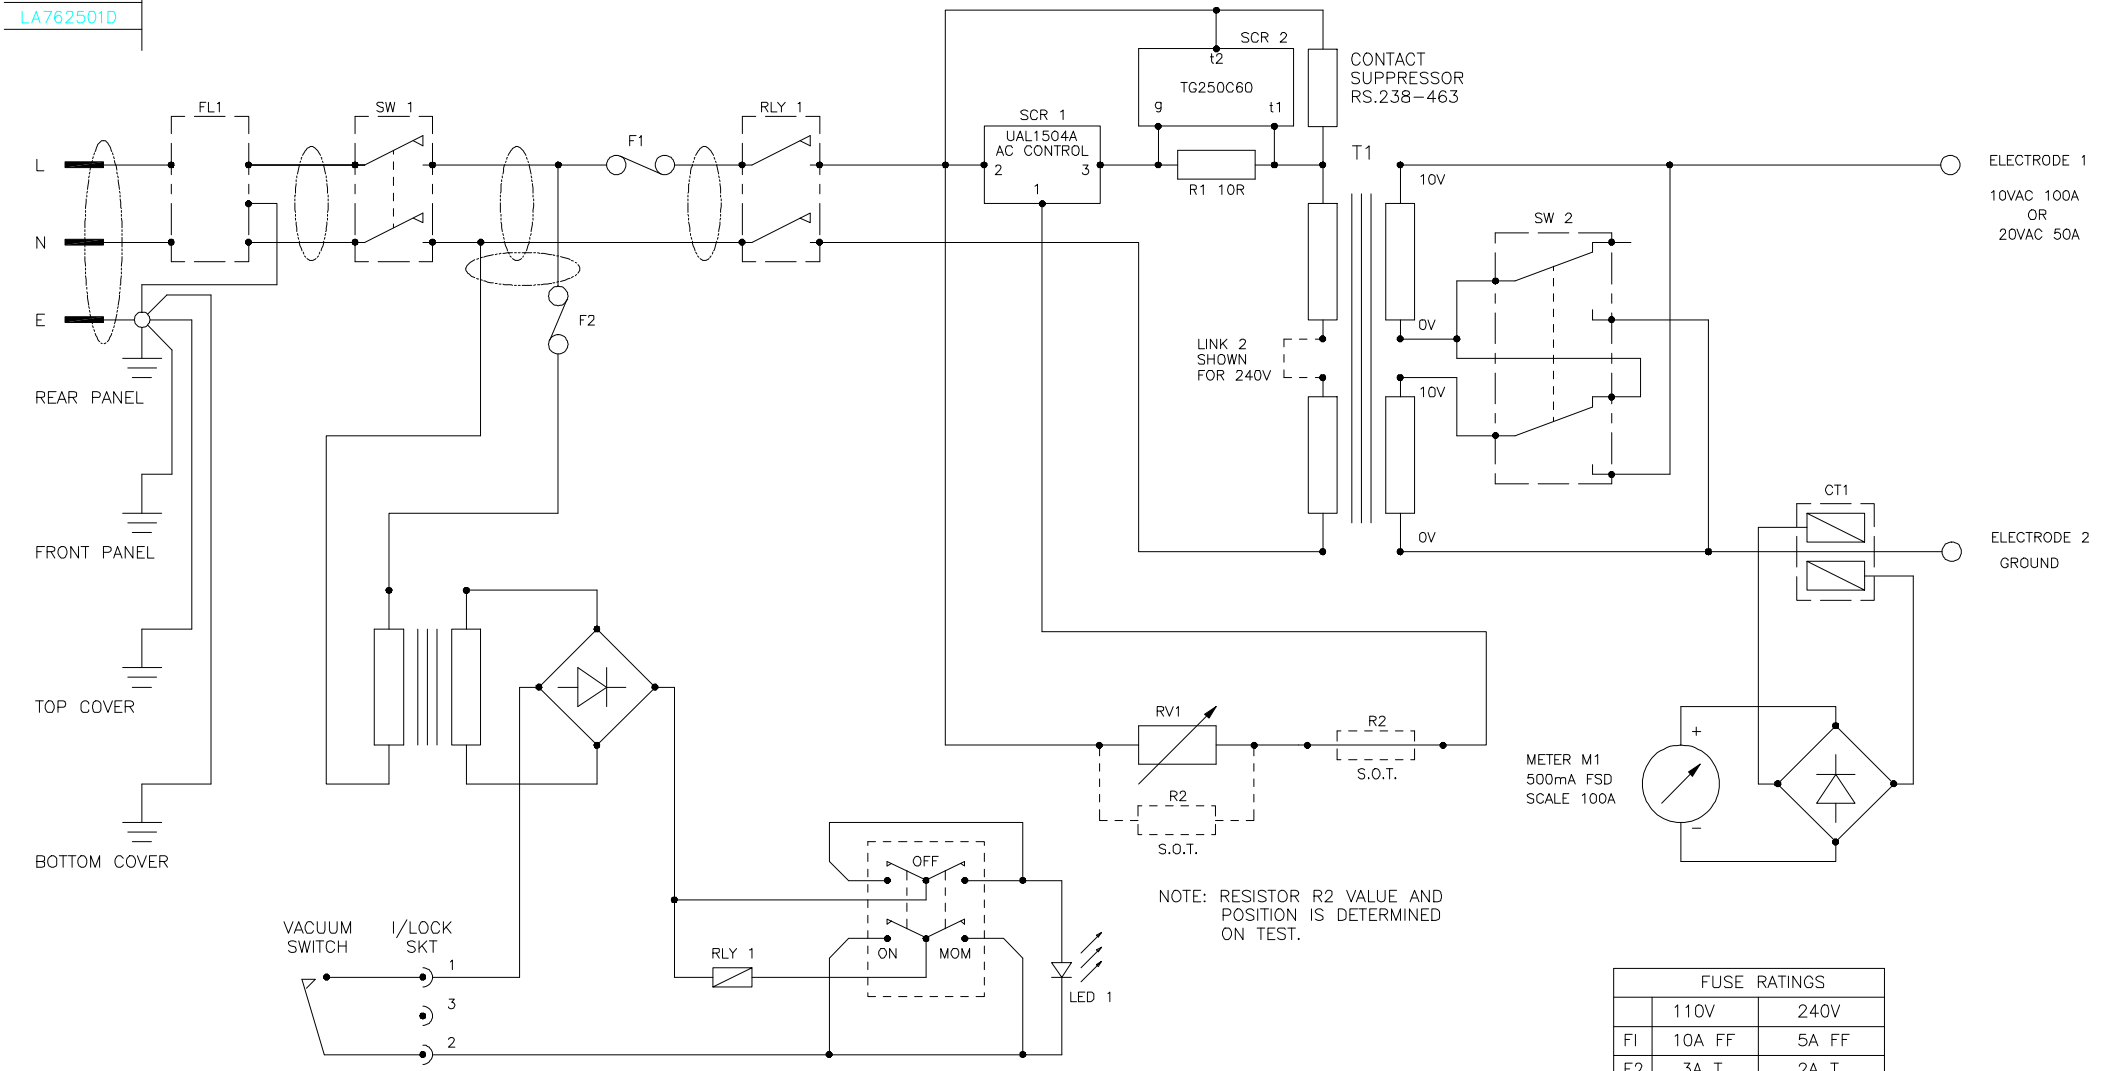

NOTE: RESISTOR R2 VALUE AND POSITION IS DETERMINED ON TEST.

FUSE RATINGS		
	110V	240V
FI	10A FF	5A FF
F2	3A T	2A T

NOTES: ALL EARTH WIRE TO BE TRI-RATED 0.75mm² (24/0.2).
MAINS CABLE TO BE DOUBLE INSULATED, ROUTED SEPERATELY FROM SIGNAL CABLES.

0 1 2 3 4 5 10 15 20

THIS DRAWING HAS BEEN CREATED USING CAD

SHEET SIZE A2

DO NOT SCALE DRAWING | REMOVE ALL BURRS | FOR EXPLANATION OF DIMENSIONS, TOLERANCE, NOTES ETC.SEE BS 308 (MECHANICAL) OR BS 3939 (ELECTRONICS)

UNLESS OTHERWISE STATED DIMENSIONAL TOLERANCE:- 0 ± 1mm, 0.0 ± 0.2mm, 0.00 ± 0.1mm
GEOMETRICAL FORM TO BE WITHIN ABOVE DIMENSIONAL TOLERANCE.
ANGULAR TOLERANCE ± 0° 30'
DRILLED HOLE ± 0,05mm
SURFACE FINISH 1.6um
DIMENSIONS IN MILLIMETERS

PROJECTION | IF IN DOUBT - ASK

MATERIAL | FINISH

QUORUM TECHNOLOGIES, NEWHAVEN,EAST SUSSEX, UK.

MODIFICATION	DATE	ISS	MODIFICATION	DATE	ISS		
						ENG	D.J.C
						DRN	D.J.C
						PASSED	
			ORIGINAL	28.2.02	1	APP'D	D.J.C

SCALE 1:1

TITLE CA7625 WIRING DIAGRAM

DRAWING No. HF762501C 1 OF 1

THIS DRAWING AND ANY INFORMATION OR DESCRIPTIVE MATTER SET OUT HEREON ARE THE CONFIDENTIAL AND COPYRIGHT PROPERTY OF QUORUM TECHNOLOGIES AND MUST NOT BE DISCLOSED. LOANED. OR COPIED IN WHOLE OR PART OR USED FOR MANUFACTURING. TENDERING. OR FOR ANY OTHER PURPOSE WITHOUT THEIR WRITTEN PERMISSION.